

Monitoring structure rebuild (thixotropy) following extrusion from a bottle, tube or spray head



RHEOLOGY AND VISCOSITY

Introduction

Many consumer products are packaged in tubes or bottles where product application involves pumping the product through a nozzle. Such products tend to be shear-thinning products where the viscosity drops during the extrusion process due to the increasing shear rate, and then recovers on exiting the orifice as the shear rate is reduced. The shear rate encountered during this process is related to the radius, r of the orifice and the volumetric flow rate Q by the following expression:

$$\dot{\gamma} = \frac{Q}{\pi r^3} \left[3 + \frac{1}{n} \right]$$

The parameter n is the power law index, which is 1 for a Newtonian liquid and between 0-1 for a non-Newtonian fluid. This value can be readily attained from a variable shear rate test by fitting a power law model to the resultant data.

By measuring the volumetric flow rate (volume dispensed in given time) and the internal radius of the orifice, it is possible to estimate the shear rate encountered during extrusion.

Because many consumer products including foodstuffs, coatings and toiletries/cosmetics can have very delicate microstructures, these structures are easily broken down during the extrusion process and may not recover their original structure until a finite time has passed. Materials which have a time-dependent structural recovery or rebuild are termed thixotropic. By calculating the shear rate encountered during extrusion and using this in the intermediate stage of a step strain-shear rate test it is possible to mimic structural breakdown resulting from extrusion.

By immediately following structural recovery through the elastic modulus G' as a function of time it is possible to determine structural recovery of the system and ultimately the structural integrity of the product at time of use. This can be important in terms of physical appearance (slump resistance), in use texture or product functionality, for example the ability to cling on to a vertical surface.

Experimental

- The structural recovery properties of toothpaste and a hair gel were evaluated under shear rate conditions associated with product extrusion during use
- Rotational rheometer measurements were made using a Kinexus rotational rheometer with a Peltier plate cartridge and a roughened parallel plate measuring system¹, and using standard pre-configured sequences in the rSpace software.
- A standard loading sequence was used to ensure that both samples were subject to a consistent and controllable loading protocol.
- All rheology measurements were performed at 25°C.
- The relevant extrusion shear rates were automatically calculated as part of the test sequence using inputted values of extruded volume, extrusion time and aperture radius. The test was programmed to use this calculated value as the intermediate shear rate in a step shear rate test with step 1 and step 2 employing a constant strain value within the samples LVER at a frequency of 1Hz.
- The time to recover 90% of the products original elasticity (G') was automatically determined and reported at the end of the test.

Results and Discussion

The automatic calculator evaluated the shear rate in the extrusion process to be 86s^{-1} for the toothpaste and 240s^{-1} for the hair gel. These values were used in the intermediate shear rate stage of the test.

Figure 1 shows the results for the toothpaste. Clearly this is a highly thixotropic material as observed from the recovery curve which shows it does not fully recover its structure in the timescale of the test, reaching only 50% of its original value of G' after approximately 500 seconds.

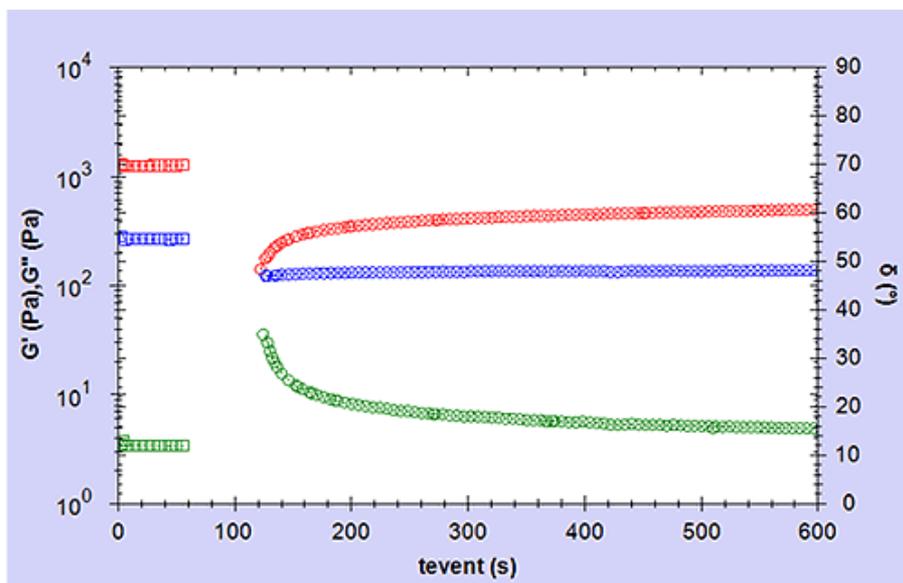


Figure 1 – Step strain/shear rate curves for a toothpaste (Elastic Modulus G' in red; Viscous Modulus G'' in blue; phase angle δ in green)

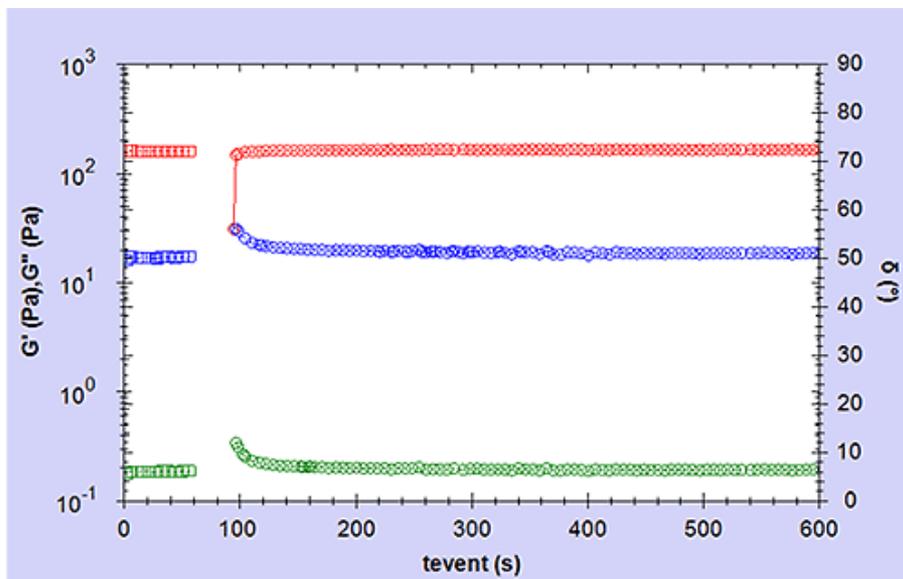


Figure 2 – Step strain/shear rate curves for a hair gel (Elastic Modulus G' in red; Viscous Modulus G'' in blue; phase angle δ in green)

Conversely, the hair gel recovers its structure almost instantaneously with 90% of recovery occurring in the first 5 seconds and completes recovery within 20 seconds. This is important for this product as it needs to provide instantaneous hold to the hair before the resin can form an elastic film for longer-term hold.

Note both materials appear to show yield stress behavior at the frequency measured since G' exceeds G'' indicating an interconnected or solid-dominant microstructure.

Conclusion

A three-step strain/shear rate test was performed on a toothpaste and hair gel to evaluate the rate and extent of elasticity recovery following extrusion from a tube. The toothpaste was shown to be highly thixotropic taking 500 seconds to recover 50% of its original elasticity while the hair gel recovered almost immediately.

Notes

- Note that testing is recommended to be undertaken with cone and plate or parallel plate geometry – with the latter being preferred for dispersions and emulsions with large particle sizes. Such material types may also require the use of serrated or roughened geometries to avoid artefacts relating to slippage at the geometry surface.



Malvern Instruments Limited
Groewood Road, Malvern,
Worcestershire, UK. WR14
1XZ

Tel: +44 1684 892456
Fax: +44 1684 892789
www.malvern.com

Malvern Instruments is part of Spectris plc, the Precision Instrumentation and Controls Company.

Spectris and the Spectris logo are Trade Marks of Spectris plc.

spectris

All information supplied within is correct at time of publication.

Malvern Instruments pursues a policy of continual improvement due to technical development. We therefore reserve the right to deviate from information, descriptions, and specifications in this publication without notice. Malvern Instruments shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance or use of this material.

Malvern Instruments owns the following registered trademarks: Bohlin, FIPA, Insitex, ISYS, Kinexus, Malvern, Malvern 'Hills' logo, Mastersizer, MicroCal, Morphologi, Rosand, 'SEC-MALS', Viscosizer, Viscotek, Viscogel and Zetasizer.